

**SPECIFICATIONS:**

The medical gas Retro-Fit outlet shall be an Amico **Alert-1** series.

Outlets shall be equipped with a primary and secondary check for positive pressure for gas services. The secondary check valve shall be rated at a minimum 200 psi [1,379 kPa] in the event the primary check valve is removed for maintenance. Outlet bodies shall be gas specific by indexing each gas service to a gas specific single pin indexing arrangement on the respective identification module.

A large color coded front plate shall be used for ease of gas identification and aesthetic appeal.

A one piece filler plate shall cover the outlet. With the back rough-in mounted the outlet shall adjust from 1/2" [13 mm] to 1" [25 mm] variation in wall thickness.

The latch-valve assembly shall be Ohmeda Diamond™ (Ohio Medical) Quick Disconnect compatible and accept only corresponding Ohmeda type gas specific adapters or any of the compatible outlets manufactured by Amico.

Amico products comply with NFPA-99.



**FEATURES:**

- Flow rate exceeds the requirements of NFPA and CSA.
- Accepts Ohmeda Diamond™ gas specific adapters.
- 100 % hydrostatic testing of each outlet and cleaned for medical gas service.
- Indexed to eliminate interchangeability of gas services.
- 1/2" [13 mm] to 1" [25 mm] wall thickness adjustment.
- Universal rough-in assembly to accept Quick Disconnect or DISS front adapters. (Can be interchanged at any time).

**PROJECT:**

---




---



---

## D I M E N S I O N S

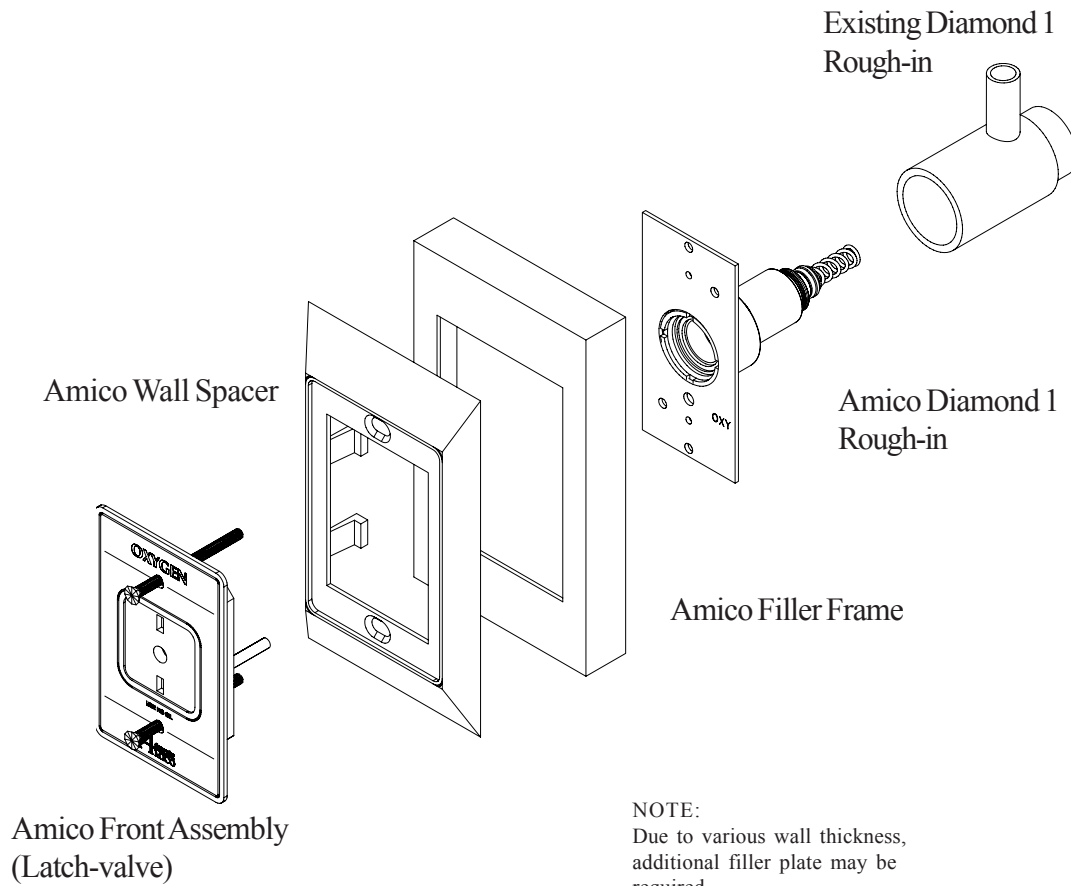

NOTE:  
Due to various wall thickness,  
additional filler plate may be  
required.

## M O D E L   N U M B E R S

<b>Amico Front Assembly</b>	<b>= O-FC01-QD-L-GAS</b>
<b>For example USA Oxygen</b>	<b>= O-FC01-QD-U-OXY</b>
<b>Amico Filler Frame</b>	<b>= O-CON-FIL-OH1-1</b>
<b>Amico Wall Spacer</b>	<b>= O-TRIM-M325C</b>
<b>Amico Diamond 1 Rough-in</b>	<b>= O-VC-OH1-L-GAS</b>
<b>For example USA Oxygen</b>	<b>= O-VC-OH1-U-OXY</b>

D I S T R I B U T E D   B Y :